




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61N 1/05	A1	(11) International Publication Number: WO 99/36122 (43) International Publication Date: 22 July 1999 (22.07.99)
<p>(21) International Application Number: PCT/US99/01021</p> <p>(22) International Filing Date: 19 January 1999 (19.01.99)</p> <p>(30) Priority Data: 09/009,247 20 January 1998 (20.01.98) US</p> <p>(71) Applicant: MEDTRONIC, INC. [US/US]; 7000 Central Avenue N.E., Minneapolis, MN 55432 (US).</p> <p>(72) Inventors: GIELEN, Frans, L., H.; Klompenstraat 10, NL-6251 NE Eckelrade (NL). DUYSENS, Victor, P., J.; Nieuwstraat 43, NL-6127 BA Brevenbicht (NL). GIJSBERS, Johan, F., M.; Fonielsweg 13, NL-6151 EH Munstergeleen (NL).</p> <p>(74) Agents: KINGHORN, Curtis, D. et al.; Medtronic, Inc. MS301, 7000 Central Avenue NE, Minneapolis, MN 55432 (US).</p>		<p>(81) Designated States: European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</p> <p>Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i></p>

(54) Title: TARGET LOCALIZATION LEAD FOR STEREOTACTIC BRAIN SURGERY

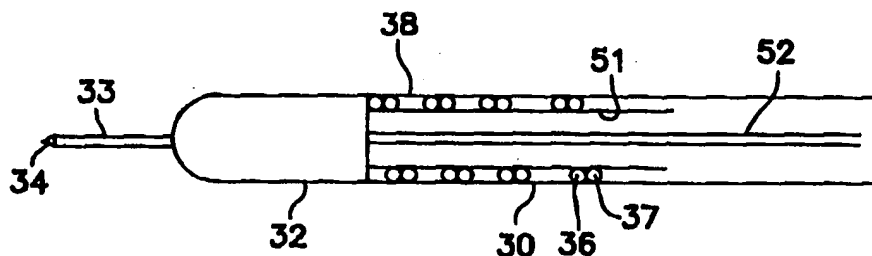

(57) Abstract

There is described a lead (30) for brain target localization in functional stereotactic brain surgery, the lead having at its distal end a micro-electrode (34) for use in recording single cell discharge patterns so as to identify functional boundaries between brain structures; and a macro-electrode (32) for delivering test stimulation for determining target location for optimal therapeutic benefit and minimum side effects. The macro-test stimulation electrode (32) is carried at the end of the lead length, and has a conventional surface area in the range of 1-20 mm² for stimulating chronic stimulation conditions. The micro-electrode (34) is positioned at the distal end of an axially aligned probe which extends distally from the macro-electrode, and has a surface area adapted to enable a single cell recording; e.g., between 0.01 and 1000 m². In an alternate embodiment, the tip micro-electrode is retractable so that the lead can be used for chronic brain stimulation.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

TARGET LOCALIZATION LEAD FOR STEREOTACTIC BRAIN SURGERY.

Field of the Invention

5 This invention relates to a lead and method for brain target localization and, more particularly, a lead for combining a micro-electrode for single cell recording and a macro-test stimulation electrode for evaluation of an optimal site for placement of the chronic cranial stimulation electrode.

BACKGROUND OF THE INVENTION

10 Systems for providing electrical stimulation to an identified location in the brain for specific therapies are coming into increased use for various purposes. Specifically, such systems have been used for treating Parkinson's Disease Tremor and Essential Tremor. A typical electrical brain stimulation system comprises a pulse generator operatively connected to the brain by a lead. The lead
15 has one or more stimulating electrodes at its distal end, designed to be implanted within the patient's brain at a precise location, so that the electrode or electrodes are optimally and safely positioned for the desired stimulation. Reference is made to U.S. Pat. No. 5,464,446, "Brain Lead Anchoring System," assigned to Medtronic, Inc., which is incorporated herein by reference, and which illustrates an effective
20 lead anchoring system and discloses a method of positioning the stimulating lead so that the electrodes are at the desired stimulation site. The lead is positioned using a stereotactic instrument, which permits a very precise movement, e.g., ± 1 mm, within the brain.

25 This invention addresses the initial step in functional stereotactic surgery, which is the localization or mapping of functional brain structures. It is to be noted that in many cases of Parkinson's Disease and Essential Tremor, the target is relatively easy to find, so that precise localization may not be necessary. However, other brain targets, such as in cases of advanced Parkinson's Disease, require the localization step. Generally, whenever the target is relatively new, in
30 the sense of lacking statistical data which reliably identifies the target location, it is necessary to first determine where, within the boundary of the functional target area, stimulation can be delivered which is effective and which does not cause problems.

35 Therapeutic benefit and non-desired effects of brain lesioning and chronic neuromodulation depend critically on this localization procedures. This procedure involves three primary steps. First, anatomical localization of brain

targets is determined using anatomical brain atlases, imaging by means of positive contrast x-rays, CT or MRI under stereotactic conditions. Thus, standard imaging techniques are used to make a first determination of coordinates for the lead's target. Next, electrophysiological identification of functional boundaries between brain structures is carried out by means of single cell recording of characteristic cell discharge patterns. This procedure requires use of an electrode which is small enough to differentiate single cells, and thus requires a micro-electrode with a very small surface area, e.g., less than one square micro-meter. The third step involves electrical test stimulation within determined functional brain structures, for the final evaluation of the efficacy of the location. Test stimulations are necessary to determine (1) efficacy of stimulation in the identified functional brain structure; and (2) any side effects caused by stimulation of the brain in this area. If the stimulation electrode is too close to the boundary of the functional brain structure, the function of adjacent brain structures will be modulated, which may lead to undesired side effects. The test stimulations are clinically most relevant when done with an electrode or electrodes with a similar surface area to that of the chronic implantable electrodes, e.g., in the range of about 1-20 square milli-meters.

As currently performed, the second and third steps, namely identification of functional boundaries with a micro-electrode and test stimulation with a larger, or macro-stimulation electrode, require first placement of the micro-electrode, withdrawal of same and then placement of the macro-electrode. These replacements require extra penetrations of the brain tissue, and therefore increase the risk of intra-cranial hemorrhages with severe permanent disability as a potential consequence. It has not been possible to perform effective test stimulation with the micro single cell electrode, because the volume of brain tissue that can be stimulated with the micro electrode is in general insufficient to evaluate efficacy and side effects. For example, our evaluation of functional stereotactic implantation of the Sub-Thalamic Nucleus (STN) or the Globus Pallidus Internae (GPi) reveals a discrepancy between electrical test stimulation with the micro single cell recording electrode and electrical stimulation with a chronic stimulation electrode. This discrepancy is most likely due to the very large difference of the electrode surface area, i.e., less than 1 square micro-meter vs. 1-20 square milli-meters, and the directly associated current density which results in stimulation of largely different volumes of cells, and therefore results in different therapeutic effects and side effects.

SUMMARY OF THE INVENTION

It is an object of this invention to provide a lead for use in functional stereotactic surgery for localization of functional brain structures, which combines a micro-electrode for identification of functional boundaries between brain structures and a macro-electrode for carrying out electrical test stimulation within functional brain structures. The macro-test stimulation electrode is positioned at the distal end of the lead casing, and has a conventional electrode surface area for stimulating electrodes in the range of about 1-20 square milli-meters. The micro-electrode is positioned at the distal end of a very narrow probe which extends distally from the macro-electrode, the micro-electrode being positioned on the tip end of the probe and having an electrode surface less than about 1000 square micro-meters, and preferably less than 1 square micro-meter. In an alternate embodiment, the micro-electrode is attached to a stylet which can be withdrawn after the localization procedure, enabling chronic use of the lead for brain stimulation.

In the use of the combined electrode lead of this invention, the lead is inserted into positions for single cell recordings by the micro-electrode, which recordings are not disturbed by the tissue displacement caused by the macro-test stimulation electrode also carried on the lead, proximally to the micro-electrode. Following each recording by the micro-electrode, a test stimulation is performed with the macro-electrode; the lead is advanced through the functional area of interest until all required recordings and test stimulations are performed, such that no subsequent brain penetration is required to complete the localization procedure.

BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 is a system diagram showing a lead in accordance with this invention having its proximal end connected to a stimulator and recorder, the lead being in position so that single cell recordings and test stimulation can be carried out for locating the site for optimum chronic brain stimulation.

Figure 2 is a schematic diagram of the distal end of the lead of this invention, illustrating the micro-electrode and macro-electrode.

Figure 3 is a schematic illustration of trajectories taken by the distal end of the lead for recording and test stimulating.

Figure 4 is a flow diagram showing the primary steps taken in using the combined electrode lead of this invention for making single cell recordings and carrying out electrical test stimulation.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

5 Referring now to Figure 1, there is shown a schematic diagram of a brain lead 30, of the type of this invention, being held in position by a stereotactic instrument. The stereotactic instrument is a commercially available device, and has a frame shown partially at 40. The frame carries a lead holder assembly indicated at 41, which in turn supports a lead holder 42. The lead 30 is positioned through the lead holder and through the guide tube as shown at 44. A micro-positioner, shown
10 schematically at 45, is used to advance the lead one cell at a time. The distal end of the lead is shown schematically to have a first larger, or macro-electrode 32 at the lead distal end, and distal to that a micro-electrode 34. As illustrated, the distal end of the lead is inserted through a burr hole in the skull of the patient, illustrated diagrammatically by BH. The proximal end of the lead is connected to an
15 appropriate stimulator and recorder, as illustrated diagrammatically at 46. The technique for positioning a cranial lead with a stereotactic instrument is well known in the art.

Referring now to Figure 2, there is shown an exploded detailed view
20 of the far distal end of a lead 30 in accordance with this invention. As illustrated, a macro-electrode 32 is positioned at the distal end of the casing 38. Electrode 32 may have the shape and surface area of a conventional cranial stimulus electrode, the surface area preferably being in the range of 1-20 mm². Extending axially distal from electrode 32 is a thin probe 33, terminating in a micro-electrode 34, having a
25 surface area less than 1000 m², and preferably less than 1 m². For example, electrode 34 may have a surface area of 500-100 m² for a semi-micro-electrode, and a surface area less than 1 m² for a micro-electrode e.g., 0.01 m². The length of probe 33, i.e., from the distal-less surface of electrode 32 to the micro-electrode 34, is suitably in the range of 1 to 10 mm, and preferably about 2-5 mm. The length of
30 this probe is important, as it establishes the distance between the two electrodes. This distance is important, since the larger electrode 32 should be sufficiently remote so that its penetration does not perturb the cells that are being probed by micro-electrode 34. Conductors 36, 37 are illustrated as coils which connect from the proximal end of the lead to electrodes 32, 34 respectively; electrode 34 is
35 electrically connected through the interior of probe 33. Tube casing 38, made of conventional biocompatible material, encapsulates the length of the the lead in a

known manner. Insulating sleeve 51 retains the coils, establishing an axial lumen. As illustrated, a stylet 52, suitably made of tungsten, connects mechanically to probe 33, so that the micro-tip electrode 34 can be withdrawn.

5 The lead is, in the preferred embodiment, designed for use only as a test lead, and thus does not need to be designed for permanent implantation. Material choices are a function of whether the lead is to be resterilized, or disposable after one patient use. The macro-electrode 32 can be made of typical acute stimulation electrode material, e.g., stainless steel, Pt Ir, or Pt. The micro-electrode needs to be durable for at least one trajectory, as described below, but
10 preferably 1-10 trajectories; the electrode material can be, e.g., tungsten, Pt Ir, or Ir. The lead must be stereotactically rigid, and of sufficient length to reach the target area of the brain. Since the radius of a typical stereotactic frame is 190 mm, and the lead needs the ability to go further to reach the target with a margin of safety, the lead should be greater than about 30 cm in length.

15 Referring now to Fig. 3, there is shown a diagrammatic representation of two test trajectories taken relative to a functional portion of the patient's brain, the functional portion being defined by a boundary F. Two illustrative trajectories are shown as indicated at T1 and T2. The distal end of the lead 30 is illustrated with respect to T1, with the micro-electrode 34 and macro-electrode 32 being illustrated. The line indicated as T_H indicates the distance from
20 the macro-electrode 32 at which current density delivered by a test stimulus pulse is above the threshold for stimulation. As the tip is moved along trajectory T1 indicated by dashed lines, through the functional structure, cell recordings are taken by micro electrode 34, and test stimulus pulses are delivered through macro-electrode 32. Knowing the threshold pattern and the distance between the two
25 electrodes, the physician can verify which recorded cells corresponds to good efficacy without non-wanted side effects. As can be seen, for trajectory T1, no cell locations correspond to a position where adjacent brain structure would not be stimulated. However, for trajectory T2 there is ample room within the functional structure where delivered stimulus pulses will effect the target brain area without stimulating adjacent brain structures outside of the functional area.
30

Referring to Fig. 4, there is shown a flow diagram outlining the primary steps taken in carrying out a localization procedure with the lead of this invention. At 55, the lead is positioned for a trajectory, e.g., trajectory T1 or T2
35 as indicated in Fig. 3. The lead is advanced until the micro-electrode 34 discovers the boundary F of the functional structure, i.e., there is a recording of a cell

corresponding to the functional structure involved. At 56, a cell recording is made, and then at 57 a test simulation pulse is delivered, and it is determined whether a stimulation is efficacious and without side effects. Next, it is determined whether the cell recodation indicates that a functional boundary has been passed, e.g., micro-electrode 34 has passed out of the functional structure area. If no, the lead is advanced to the next cell, as indicated at 59, by the micro-positioner 45, and the cycle is repeated. When, at step 58, the trajectory has been determined to have completed the path through the functional area, it is determined at 60 whether a new trajectory is to be done. If yes, steps 55-59 are carried out in the same manner. As indicated above, in any particular case a number of trajectories may be required, in order to find a suitable stimulus location.

Following the localization procedure at Figure 4, and determination of a suitable location for chronic stimulation, the lead can be withdrawn. In another embodiment, micro-electrode 34 may be attached to a movable stylet 52, which can be withdrawn while holding macro-electrode 32 at the target position. In such case, the lead is fixed with respect to the patient's skull in a manner as referenced above, whereafter chronic stimulation can be carried out, generating and delivering stimulus pulses through the lead and macro-electrode 32. Accordingly, the lead of this invention can be used solely as a test lead that can be disposed of after the localization procedure, or may be designed both for the test procedure and for chronic stimulation.

CLAIMS

1. A lead for brain target localization, comprising a proximal end and a distal end with a length therebetween, a casing covering the lead over said length, first and second conductors within said casing extending between said proximal and distal ends, and

a first stimulating electrode at said distal end and connected to said first conductor, said first electrode having a surface in the range of about 1-20 mm²; and

a probe element extending more than 1 mm distally from said first electrode and carrying a micro-electrode at its distal tip, said micro-electrode having a surface area in the range of 0.01 to 1000 m², and being connected to said second conductor.

2. The lead as described in claim 1, wherein said probe has a length in the range of about 1-10 mm.

3. The lead as described in claim 2, wherein said lead length is substantially cylindrical, and said probe is positioned along the center axis of said lead.

4. The lead as described in claim 3, wherein said probe is less than about 0.2 mm in thickness.

5. The lead as described in claim 1, wherein said first electrode has a cylindrical surface congruent with said lead casing.

6. The lead as described in claim 1, wherein said micro-electrode has a surface area of less than 1 m²

7. The lead as described in claim 1, wherein said micro-electrode has a surface area in the range of 500 to 1000 m².

8. The lead as described in claim 1, comprising a stylet attached to said probe element, whereby said probe element can be withdrawn from said lead.

9. The lead as described in claim 1, wherein said length is at least 300 mm.

5 10. A system for brain target localization, comprising a stereotactic instrument mountable on a patient's head, a lead comprising a proximal end and a distal end with a length therebetween for use in brain target localization, a micro-positioner for positioning said lead when held by said stereotactic instrument so that said lead distal end is movable within the patient's brain, stimulation means for delivering test stimulation pulses through said lead, and recording means for
10 recording cell discharge patterns, said lead further comprising:

a first stimulating electrode at said distal end and connected to said first conductor, said first electrode having a surface in the range of about 1-20 mm²; and

15 a probe element extending more than 1 mm distally from said first electrode and carrying a micro-electrode at its distal tip, said micro-electrode having a surface area in the range of 0.01 to 1000 m², and being connected to said second conductor.

20 11. The system as described in claim 10, wherein said micro-electrode has a surface area of less than 1 m².

12. The system as described in claim 10, wherein said micro-electrode has a surface area in the range of 500 to 1000 m².

25 13. The system as described in claim 10, comprising a stylet attached to said probe element, whereby said probe element can be withdrawn from said lead.

30 14. The system as described in claim 10, wherein said length is at least 300 mm.

15. A method for determining a site for brain stimulation within a predetermined patient functional structure, comprising:

35 providing a lead having a proximal end and a distal end and a length therebetween, the lead having first and second conductors extending between said proximal and distal ends, the lead further having a first stimulating electrode at

said distal end and connected to a first of said conductors, and a probe element extending distally from said first electrode and carrying a cell-recording electrode connected electrically to said second conductor;

positioning said lead stereotactically for moving said lead
5 along a trajectory through the patient's brain;

moving said lead along said trajectory, said moving comprising micro-positioning said lead, for taking respective cell recordings from said cell-recording electrode along said trajectory, and test stimulating through said stimulating electrode corresponding to each said cell recording; and

10 carrying out said cell recording and test stimulating along one or more of said trajectories until a satisfactory site within a patient functional structure is found.

16. The method as described in claim 15, comprising determining
15 from each said respective cell recording when said cell is within said functional structure.

17. The method as described in claim 16, comprising determining
20 from each said test stimulating whether stimulation at such position is efficacious.

18. The method as described in claim 17, comprising determining
when stimulation at about a cell location found to be within said functional structure does not adversely stimulate a brain portion outside of said brain structure.

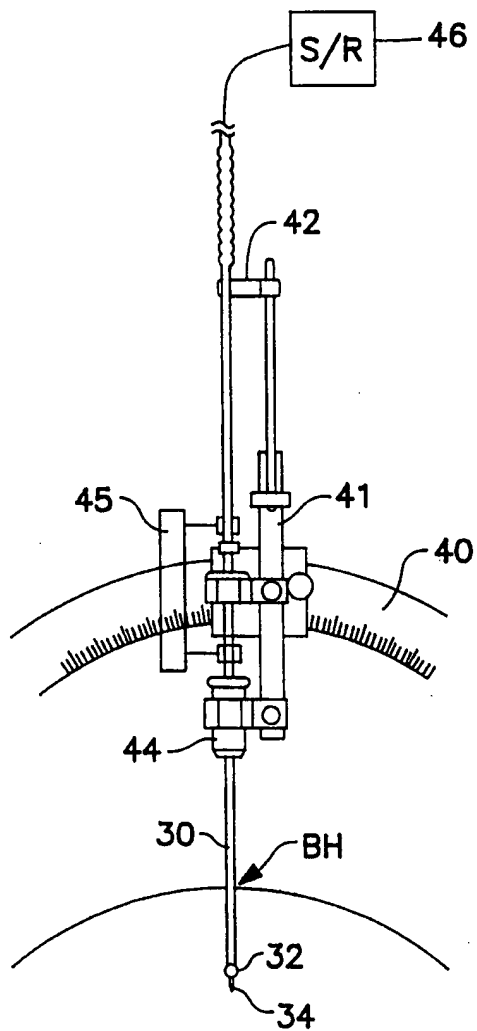


FIG. 1

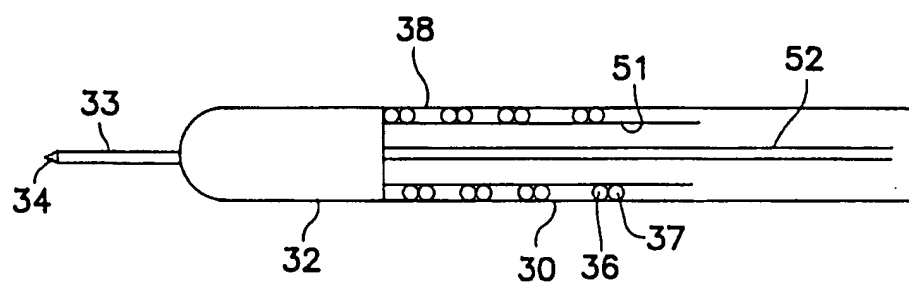


FIG. 2

3 / 3


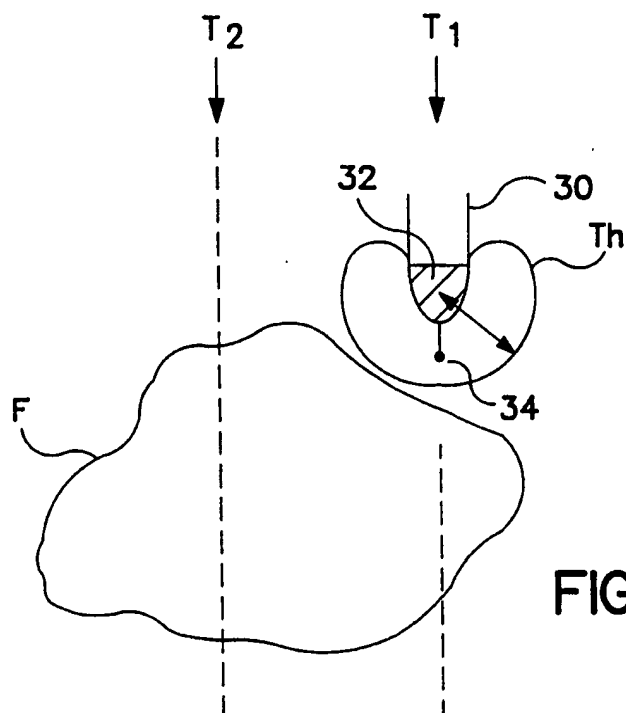


FIG. 3

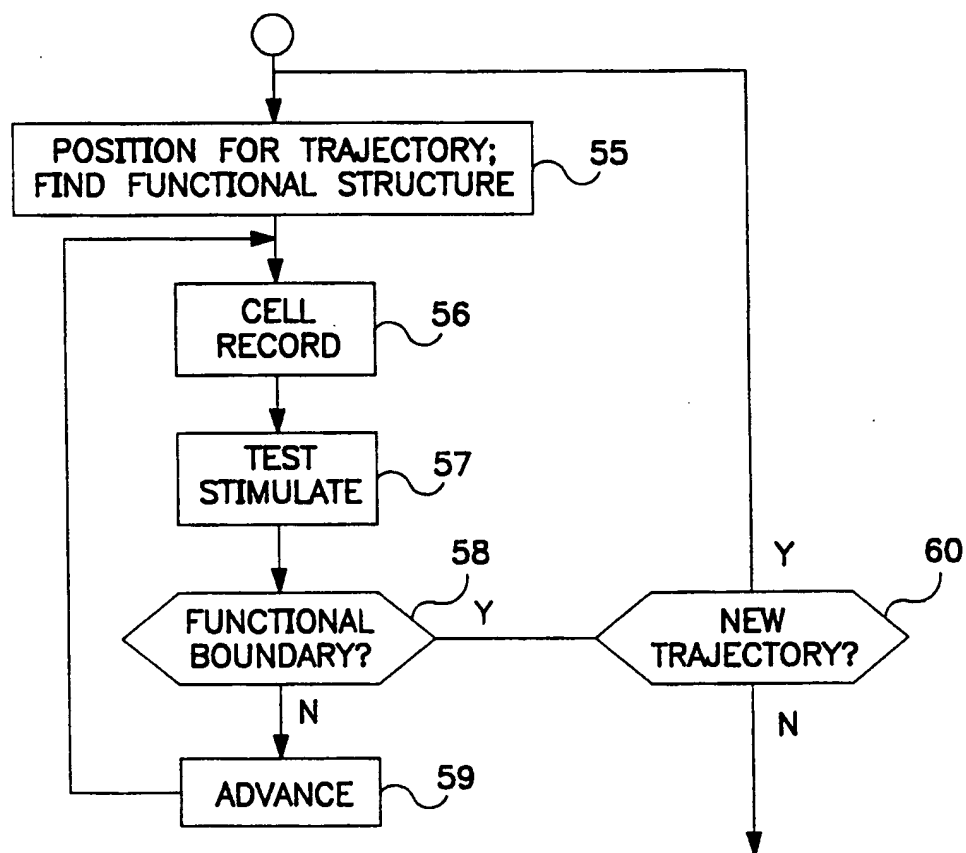

INTERNATIONAL SEARCH REPORT

Intern. Application No

PCT/US 99/01021

A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 A61N1/05

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 A61N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4 245 645 A (PICARD ROLAND ET AL) 20 January 1981 see column 4, line 11 - column 8, line 57; figures	1-7, 10-12,15
A	US 5 464 446 A (DREESSEN CHRIT ET AL) 7 November 1995 cited in the application see column 2, line 58 - column 3, line 35; figure 1	1,10,15
A	FR 2 332 743 A (INST NAT SANTE RECH MED) 24 June 1977 see page 1, line 38 - page 4, line 40; figures	1,10,15
	-/--	



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

10 May 1999

Date of mailing of the international search report

18/05/1999

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Rakotondrajaona, C

INTERNATIONAL SEARCH REPORT

Inter: nal Application No

PCT/US 99/01021

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4 681 103 A (BONER JAMES C ET AL) 21 July 1987 see column 2, line 16 - column 3, line 6; figures ---	1,10,15
A	EP 0 319 844 A (AD TECH MEDICAL INSTR CORP) 14 June 1989 see page 3, column 4, line 29 - page 6, column 9, line 9; figures -----	1,10,15

INTERNATIONAL SEARCH REPORT

...formation on patent family members

International Application No

PCT/US 99/01021

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 4245645 A	20-01-1981	CA 1065969 A	06-11-1979
US 5464446 A	07-11-1995	DE 4434741 A	13-04-1995
		JP 2707487 B	28-01-1998
		JP 7163667 A	27-06-1995
		NL 9401665 A	01-05-1995
FR 2332743 A	24-06-1977	NONE	
US 4681103 A	21-07-1987	NONE	
EP 0319844 A	14-06-1989	US 4850359 A	25-07-1989
		US 4869255 A	26-09-1989
		AT 114439 T	15-12-1994
		CA 1325831 A	04-01-1994
		DE 3852279 D	12-01-1995
		DE 3852279 T	06-04-1989